

OMNIPOD[®] 5

NOW INTEGRATED WITH DEXCOM G7

Pod and Dexcom G7 shown without the necessary adhesive.

For your current Omnipod® 5 patients interested in Dexcom G7

Easiest path to transition to G7

- 1 Continue using existing G6 Pods and supplies until "Compatible with G7" appears on their Pod refill box




- 2 Prescribe Dexcom G7 to pair at their next Pod change

Alternative pharmacy option

If your patient cannot wait, they may transfer their current Pod refill prescription to their partnered pharmacy with G7-compatible Pods

(Note: This is not the preferred path and will result in additional steps for you and your patients)

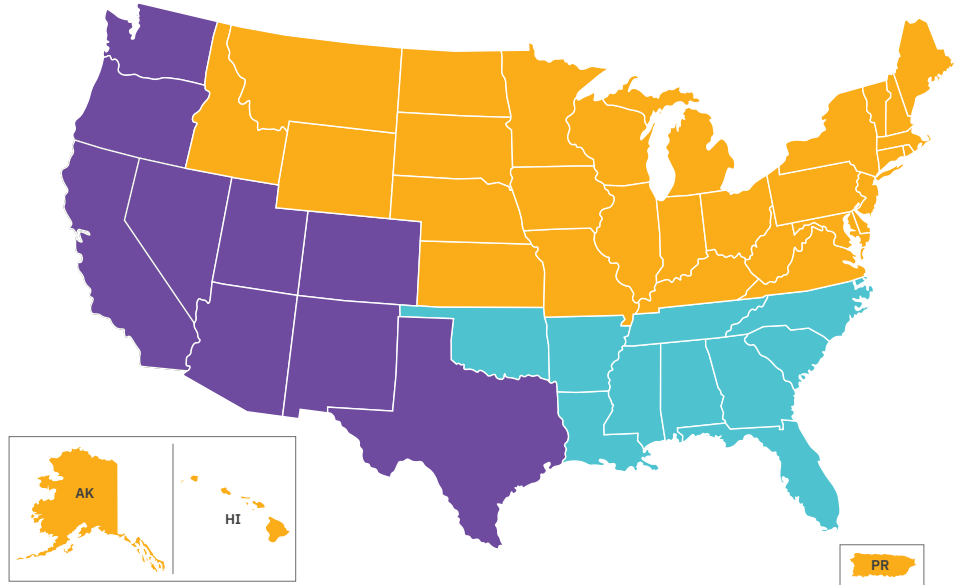

Insulet | 100 Nagog Park, Acton, MA 01720 | 1-800-591-3455 | [omnipod.com](https://www.omnipod.com)

Important Safety Information: The Omnipod 5 Automated Insulin Delivery System is indicated for use by individuals with type 1 diabetes mellitus in persons 2 years of age and older. The Omnipod 5 System is intended for single patient, home use and requires a prescription. The Omnipod 5 System is compatible with the following U-100 insulins: NovoLog®, Humalog®, and Admelog®. Refer to the Omnipod 5 Automated Insulin Delivery System User Guide at omnipod.com/safety for complete safety information including indications, contraindications, warnings, cautions, and instructions.

© 2024 Insulet Corporation. Omnipod and the Omnipod 5 logo are trademarks or registered trademarks of Insulet Corporation in the United States of America and other various jurisdictions. All rights reserved. Dexcom, Dexcom G6, and Dexcom G7 are registered trademarks of Dexcom, Inc. and used with permission. All other trademarks are the property of their respective owners. The use of third party trademarks does not constitute an endorsement or imply a relationship or other affiliation. INS-OHS-06-2024-00231 V1.0

